


Evoflex®

INSTALLATION AND USER'S INSTRUCTIONS

ART NOS. EB205, EB225, EB235 & EB275



These instructions provide important information for the safe use and maintenance of the Bodypoint Evoflex. Give these instructions to the user or their caregiver and review them to ensure that they are understood.

Optional Bodypoint belt mounting hardware may be used for mounting to wheelchairs and seating systems.

⚠ WARNING! Product should be installed and fitted by a qualified rehab technician.

USE:

⚠ WARNING! This product should only be used for positioning a person in a wheelchair or work chair. It is NOT intended for use as a transportation safety device, as a personal restraint device, or in any other application where its failure could result in injury. Misuse of this product is unauthorized and unsafe.

⚠ WARNING! This pelvic stabilizer must be worn tightly fitted across the lower pelvis or thighs at all times. A loose belt can allow the user to slip down and create a risk of strangulation. Have your seating specialist demonstrate its proper adjustment and use.

⚠ WARNING! Accidental release of this pelvic stabilizer can allow the user to slip down or fall from the wheelchair. If the user's movements or cognitive abilities could lead to accidental release, a caregiver must be present at all times during its use. Ensure that all caregivers know how to unfasten the product. Failure to do so may delay release in an emergency.

⚠ WARNING! As with any new seating support, this product may change the way a person sits. Users must continue to practice

regular pressure relief activities and skin integrity checks, not only where this product contacts the user, but also in primary pressure-bearing areas such as the sacrum, legs, and buttocks. If increased skin redness or irritation occurs, discontinue use and consult your physician or seating specialist. Failure to do so may result in serious injury, such as pressure ulcers.


MAINTENANCE: Check periodically for signs of wear in the stitching, webbing, and pads. If significant wear is found, contact your supplier for qualified repair or replacement by Bodypoint. Under no circumstance should this product be altered or repaired by unqualified persons—health and safety depend on it!

🧺🚫🧼🚫 CLEANING: Machine wash, hot, 60°C (140°F). Do not bleach. Tumble dry, low temperature, or drip dry. Do not iron. (Placing the product inside a cloth bag during washing helps prevent scratches to the product and the machine.)

WARRANTY: This product carries a limited lifetime warranty against defects in workmanship and materials arising under normal use by the original consumer. Contact your supplier or Bodypoint for warranty claims.


For more information on Bodypoint products, and a list of distributors outside the USA go to www.bodypoint.com.

 **Bodypoint®**

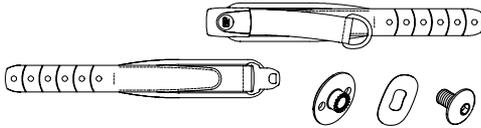



PACKAGE CONTENTS

- Evoflex Pelvic Stabilizer
- M6 x 8 screw
- M6 Low-profile flange nut
- Spring Washer

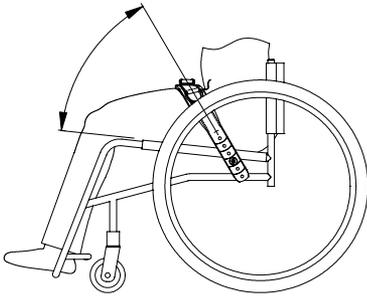



BELT POSITION

The recommended belt angle is 30°-90° from the seat, according to the positioning needs of the user. Determine the best position for the belt and, with the adjustment strap fully tightened, locate the desired anchor points, then select from the mounting methods shown.

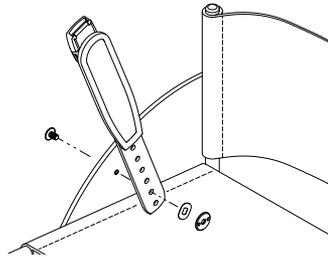



SIDE GUARD MOUNTING

Drill 6mm (1/4") hole or use existing hole/slot to attach belt using included fasteners.

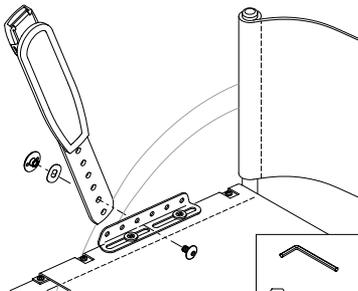

SEAT TUBE MOUNTING

(Requires Art. No. HW200-20 or -90)

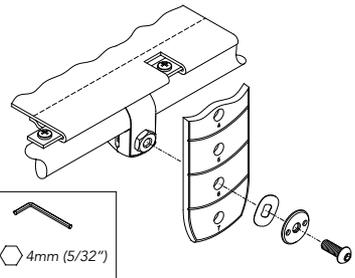


BAND CLAMP OR FRAME CLAMP MOUNTING

(Requires Art. No. HW320 or HW310)

Attach clamp to seat tube. Attach belt using the M6 screw included with the clamp.

ADJUSTMENT

To restrict belt rotation use included spring washer. Omit washer to allow for easy lateral transfers.

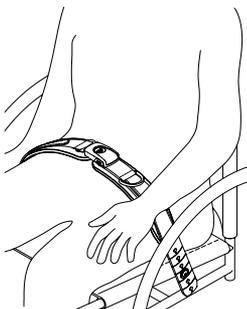

When properly adjusted and the belt tightened, it should fit snug so that the user's pelvis is secure. Tighten the D-ring pull until all slack is removed and the pads under the buckle are touching. If length adjustment is necessary to achieve a good fit or to remove the product for cleaning, this can be done at the end straps.

SAFETY CHECK

When properly positioned in wheelchair, have user lean forward and side to side to check fit. Check for:

1. Normal operation of buckle and adjustment straps.
 2. **Comfort** Look for areas of irritation.
 3. **Position** If too high or too low, adjust anchor points.
 4. **Interference with other devices** Relocate anchor points as necessary.
5. Move chair through full range of motion, including tilt, folding, and rolling. Check for any interference.